


FEHLING...

... THE DIFFERENCE

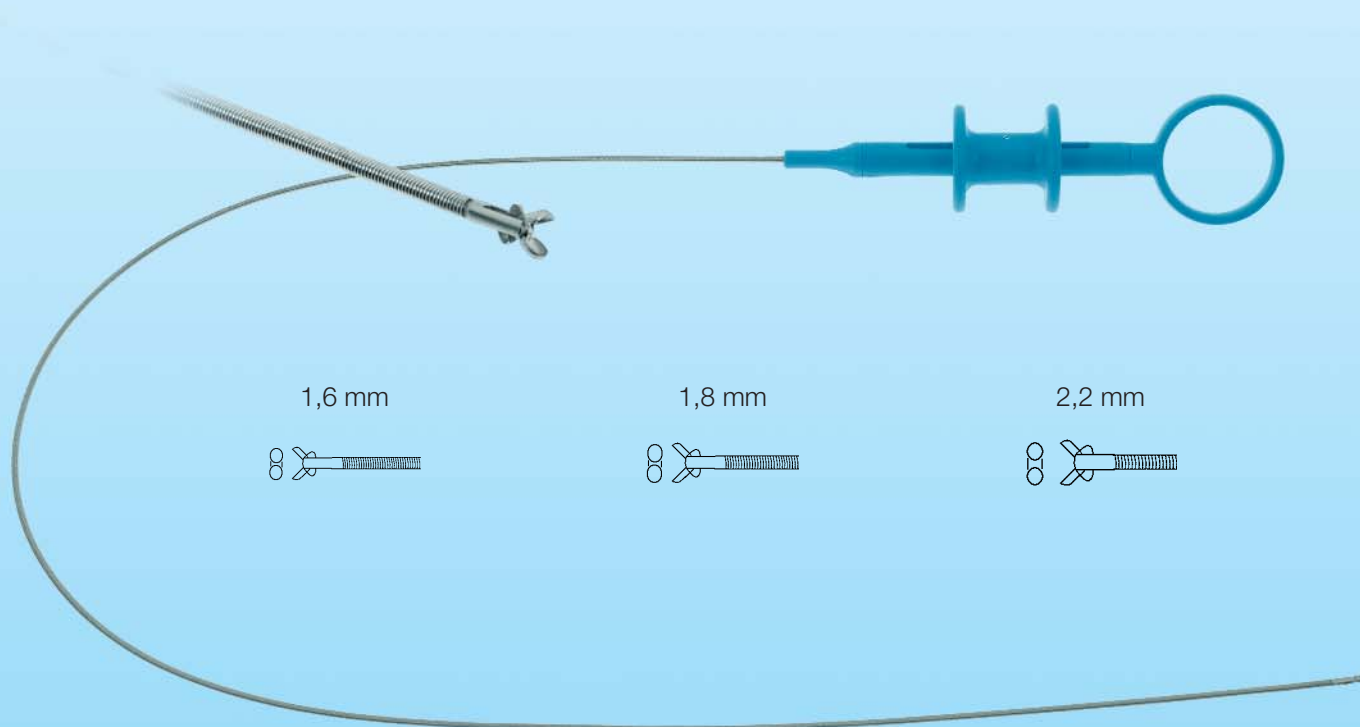

STERILE 1x BIOPSY FORCEPS STERILE 1x BIOPTOME

LENGTH OF SHAFT SCHAFTLÄNGE	CUP-DIAMETER / MAULDURCHMESSER		
	1,6 mm	1,8 mm	2,2 mm
510 mm	MOA-1	MOA-5	MOA-9
800 mm	MOA-2	MOA-6	
1000 mm	MOA-3	MOA-7	
1200 mm	MOA-4	MOA-8	MOB-1

SOFT SHAFT
WEICHER SCHAFT

510 mm		MOB-4	
1200 mm		MOB-5	

FEHLING


SURGICAL INSTRUMENTS, INC.

509 Broadstone Lane · Acworth, GA 30101

Toll Free: 1-800-FEHLING (800-3345464), Fax: 770 794-0122, E-Mail: info@fehlingsurgical.com

FEHLING...

... THE DIFFERENCE

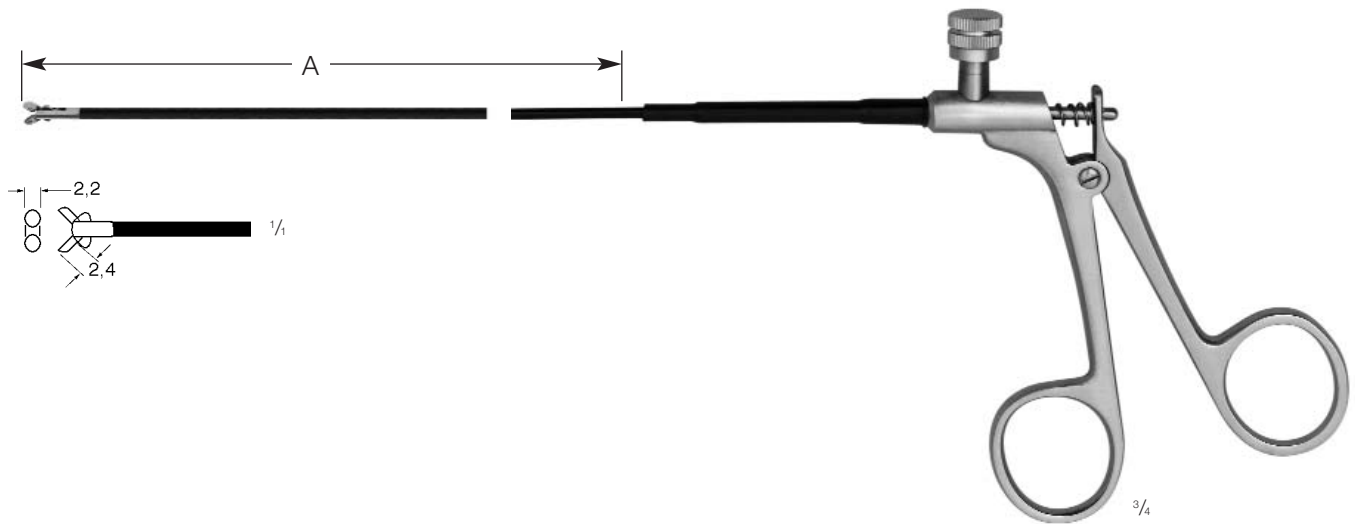

REUSABLE BIOPSY FORCEPS WIEDERVERWENDBARE BIOPTOME

CUP-DIAMETER MAULDURCHMESSER	2,2 mm
LENGTH OF SHAFT "A" SCHAFTLÄNGE "A"	ITEM NR. ART.-NR.
510 mm	MOC-1
1000 mm	MOC-2
1200 mm	MOC-3

Your Distributor
Ihr Vertriebspartner